



[www.antigentestdevice.com](http://www.antigentestdevice.com)



## Efficient Covid-19 Self Test Rapid Antigen Test

KINGSTAR INC is a leading China Efficient Covid-19 Self Test Rapid Antigen Test manufacturers, suppliers and exporter. Efficient covid-19 self test rapid antigen test is based on colloidal gold immunochromatography assay. This type tests can get results simpler and more convenient. People can do testing at home by themselves.

Find a huge selection of Efficient Covid-19 Self Test Rapid Antigen Test from China at KINGSTAR INC.

## Product Introduction

Efficient covid-19 self test rapid antigen test is intended for use by people who need to do test of covid-19. No need to go for professional medical staffs, you can operate by yourselves.

## Product Parameter (Specification)

1. Test Cassette.
2. Extraction Tube (with Extraction Solution).
3. Swab.
4. Instructions for Use.

# Efficient covid-19 self test rapid antigen test

Nasal Swab test for personal use




1 Test Cassette



1 Swab



1 Extraction Solution



1 Instructions for Use



1 Timer or Clock(Not included)



## Product Feature and Application

Efficient covid-19 self test rapid antigen test is for own usage only. It is suitable for used by people who are suspected of having a COVID-19 disease. Suitable for users over 18 years of age.



Instant result after  
15-20 minutes



Direct detection  
of the virus



Store the product  
at 2-30°C



High accuracy








Easy to use

## Product Details

Efficient covid-19 self test rapid antigen test can help you get the result around 15 minutes. DO NOT read after 20 minutes.


## Test steps

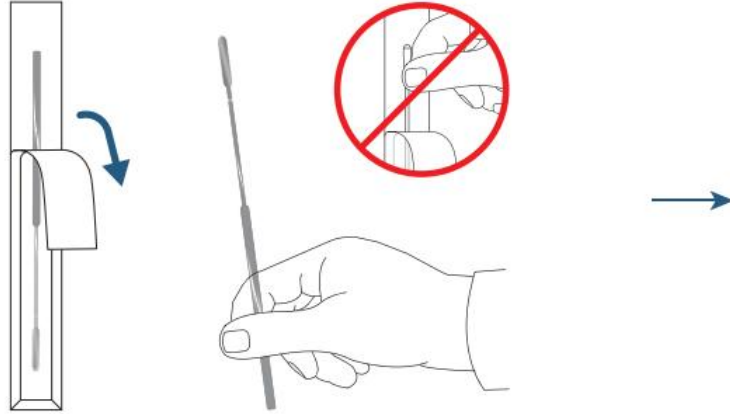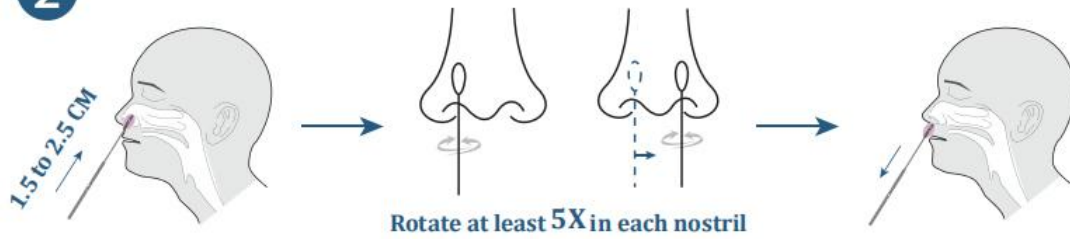**1****2**

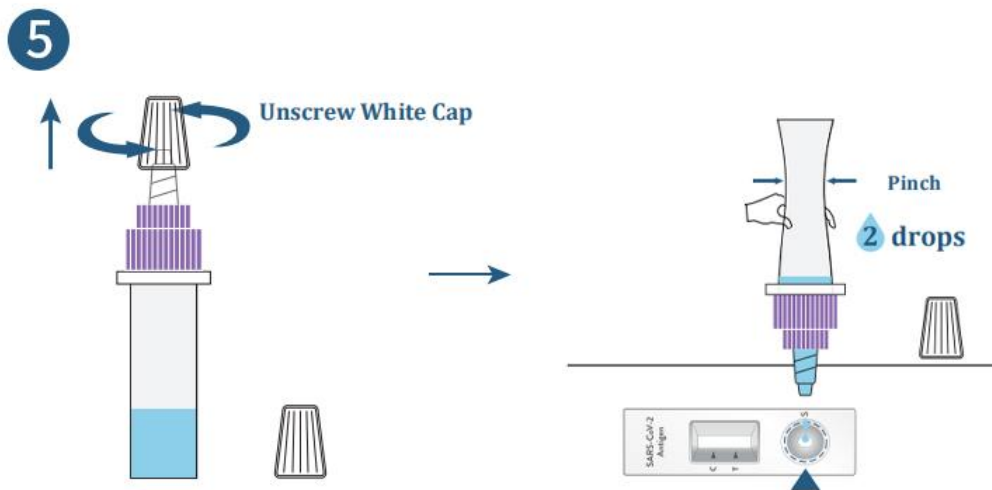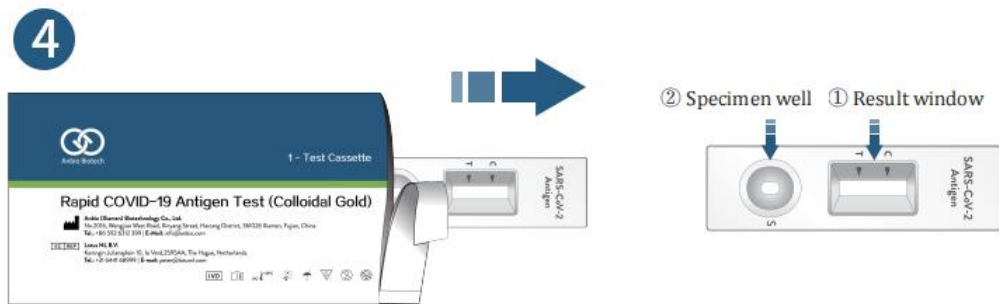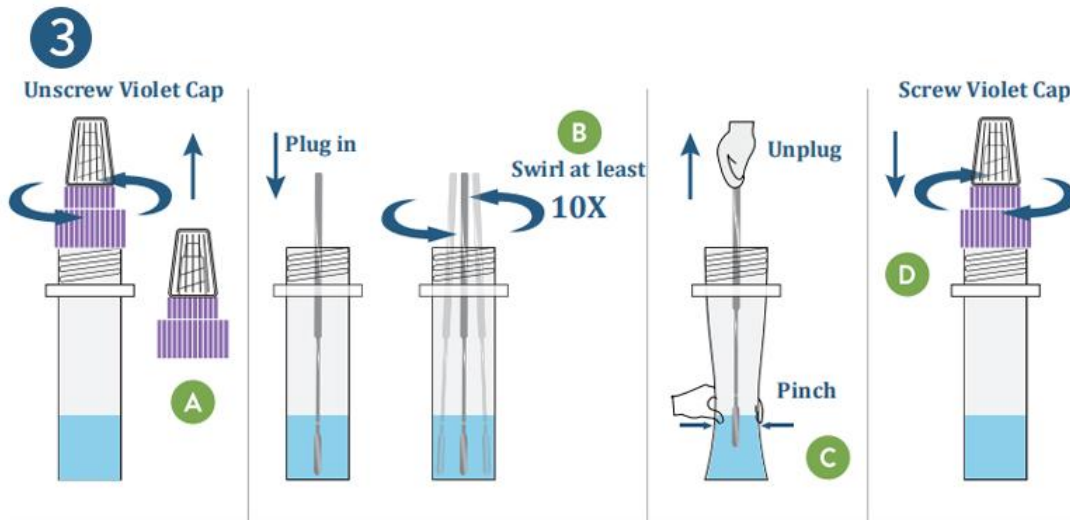

## Read the result at 15 minutes

### Interpretation of the test results

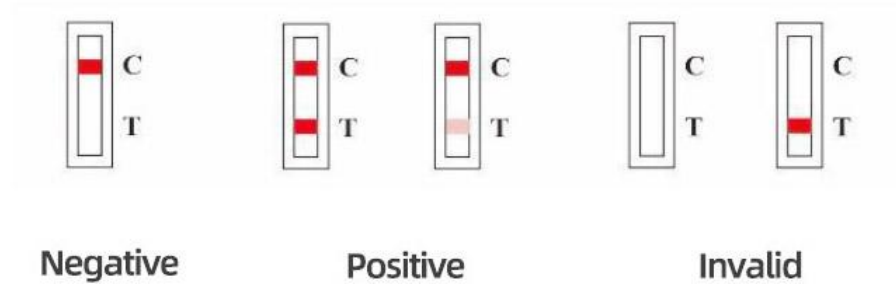

### Warning and precaution

1. For use in in vitro diagnostics.
2. Do not use this test beyond the expiration date printed on the outer carton.
3. To avoid erroneous results, samples must be processed as directed in the Test Procedure section.
4. Do not use any of the test components more than once.
5. Proper collection and storage of specimens are critical to performing this test.

### Storage and stability

1. Store the product at 2-30°C, the shelf life is months.
2. The test card should be used immediately after opening the pouch.
3. Test components must be at room temperature (15–30°C) when used to have.

We have single serving,  
five servings and 20 servings.  
(If you have specific requirement, pls let us know.)



The following is the certificates of Efficient covid-19 self test rapid antigen test.





**Anbio (Xiamen) Biotechnology Co., Ltd**  
 No. 2016, Xiang'an Road, Xiang'an District, Xiamen City,  
 P.R. China

Certification No. IT298645-1  
 Revision date: 22/06/2020

*Bureau Veritas Italia S.p.A. certifies that the Management System of the above organisation has been audited and found to be in accordance with the requirements of the management system standards detailed below*

**EN ISO 13485:2016**  
 Scope of certification

Design and manufacture of fluorescence-based immunoassay reagent and devices, as an aid in clinical assessment of cardiovascular, gastric, inflammation, diabetic and infectious diseases detection, as well as hormone, vitamin testing. Design and manufacture of IVD reagents as an aid in clinical assessment of blood type testing.

Certificate awarded in conformity with the requirements of ACCREDIA DT 02-DC Rev.00

Original cycle start date: **22/06/2020**  
 Expiry date of previous cycle: **n.a.**  
 Certification / Recertification Audit date: **17/05/2020**  
 Certification / Recertification cycle start date: **22/06/2020**

Subject to the continued satisfactory operation of the organization's Management System, this certificate expires on: **21/06/2023**

Certificate No. - Version: **IT298645-1** Revision date: **22/06/2020**

*Giorgio Lanzafame*  
**GIORGIO LANZAFAME** - Local Technical Manager



Certification body address:  
 Bureau Veritas Italia S.p.A., Viale Monza, 347 - 20126 Milano, Italia

SDQ N° 005A  
 Veritas Italia Audited to EN ISO 13485:2016 by BUREAU VERITAS Italia S.p.A. in accordance with the requirements of EN ISO 13485:2016 and ISO 9001:2015.

Further clarifications regarding the scope of this certificate and the applicability of the management system requirements may be obtained by consulting the organisation. To check this certificate validity please refer to the website [www.bureauveritas.it](http://www.bureauveritas.it)





# CERTIFICATE

**EC Certificate No. 1434-IVDD-451/2021**

**EC Design-examination  
Directive 98/79/EC concerning  
*in vitro* diagnostic medical devices**

Polish Centre for Testing and Certification certifies  
that manufactured by:

*Anna (Kingstar) Biotechnology Co., Ltd.  
No. 207A, Wuyangshan West Road, Shuangyang Street, Haining  
District, 314100 Zhejiang, P.R. China*

*in vitro* diagnostic medical devices  
for self-testing

**Rapid COVID-19 Antigen Test (Colloidal Gold) / Nasal Swab**

*A606101, A606102, A606103, A606104, A606105, A606106*

in terms of design documentation, comply with requirements  
of Annex III (Section 6) to Directive 98/79/EC (as amended)  
implemented into Polish law,  
as evidenced by the audit conducted by the PCBC

Validity of the Certificate: from 16.08.2021 to 27.05.2024

The date of issue of the Certificate: 16.08.2021

The date of the first issue of the Certificate: 16.08.2021



Issued under the Contract No. **MD-124/2021**  
Application No: 243/2021  
Certificate bears the qualified signature.  
Warsaw, 16/08/2021  
Module A1

Anna  
Małgorzata  
Wyroba

Elektronicznie  
podpisany przez  
Anna Małgorzata  
Wyroba  
Data: 2021.08.16  
10:32:41 +02'00'  
**Vice-President**  
Mgr Anna Wyroba